




State Extract Validation Information

When the “Complete PCR” process is started it will first check the “Closed Call Rules” for basic required fields, once the PCR satisfies those rules it will automatically generate the State Extract (NEMSIS 3.x) which sends the PCR to the State once it is marked complete and saved to the server. Those are extract validation rules created based on NEMSIS 3.x (Federal) and State EMSA. It **can** produce a ‘Warning’ (Yellow) or a ‘Failure’ message (Red). The screenshots below show the 2 message windows and what to do if you encounter them.

- If you encounter a ‘Warning’, click on the message field and/or correct the section described in the message window to satisfy the requirements.
 - If you are **unable** to correct the issue, click on **“Ignore and Complete”** to bypass the warning. **If this warning occurs frequently, please notify your EMS division so the warning can be addressed long term** and help to complete records. It is a warning only and may be a reminder to complete a field overlooked.
 - **Example of a Validation Warning:**

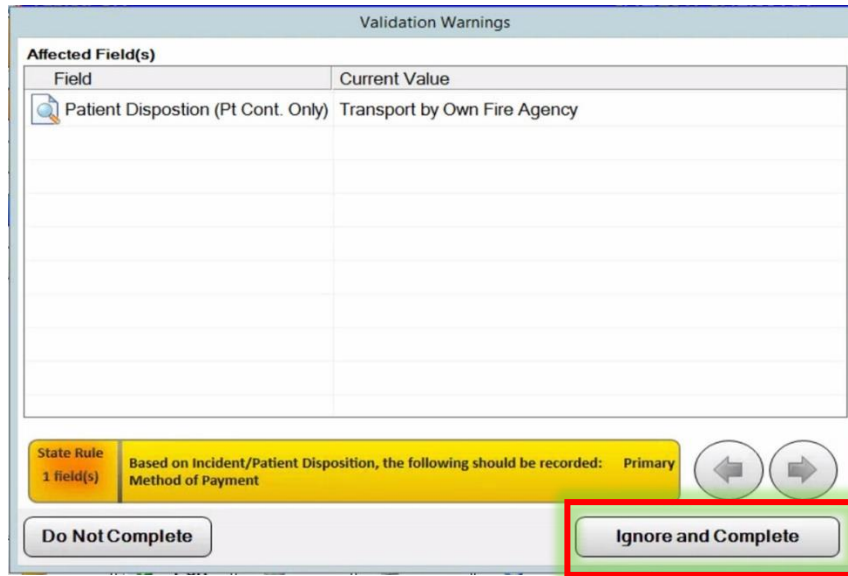

- If you encounter a Failure, click on the message field or correct the section described in the yellow message window to satisfy the requirements. You may not be able to correct the problem listed. **If you cannot** correct the problem, you can click the **“Skip State Rules”** – please notify you EMS Division as soon as possible and provide the basic call information with a description of the error, if possible a screenshot of the error message so it can be corrected in the system.
 - Click on the button next to the RED ‘X’ to open the “Validation Failure” window with the messages.

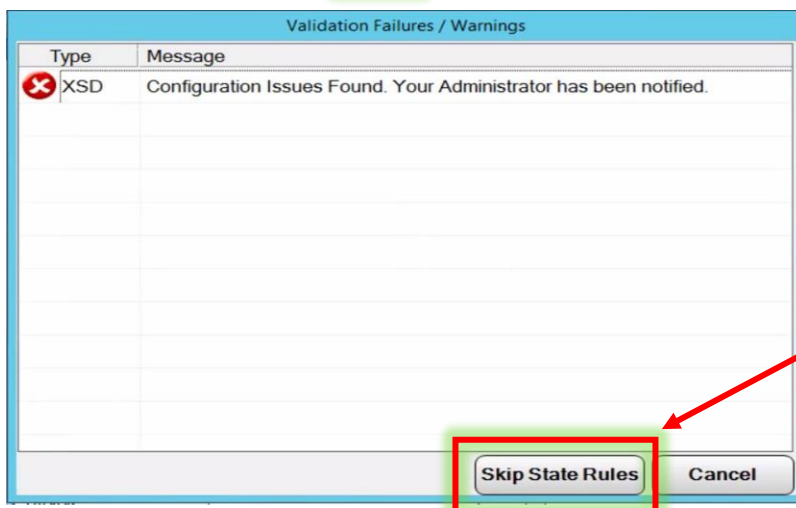

Click on **“Skip State Rules”** button to bypass and complete the PCR **only** if you are unable to correct the issue displayed.